


## EDXRF Sulfur Analyzer

# rx-630SA

### Operability improved by adoption of 5" color touch screen.

Thanks to the new GUI, operator can measure sulfur content precisely without training.

rx-630SA determines total sulfur in petroleum products, such as gas oil, fuel oil, crude oil and naphtha, using energy dispersive X-ray fluorescence(EDXRF) method, which is an accurate, non-destructive, economical and yet quick method prescribed in ISO 8754 and ASTM D4294-03.

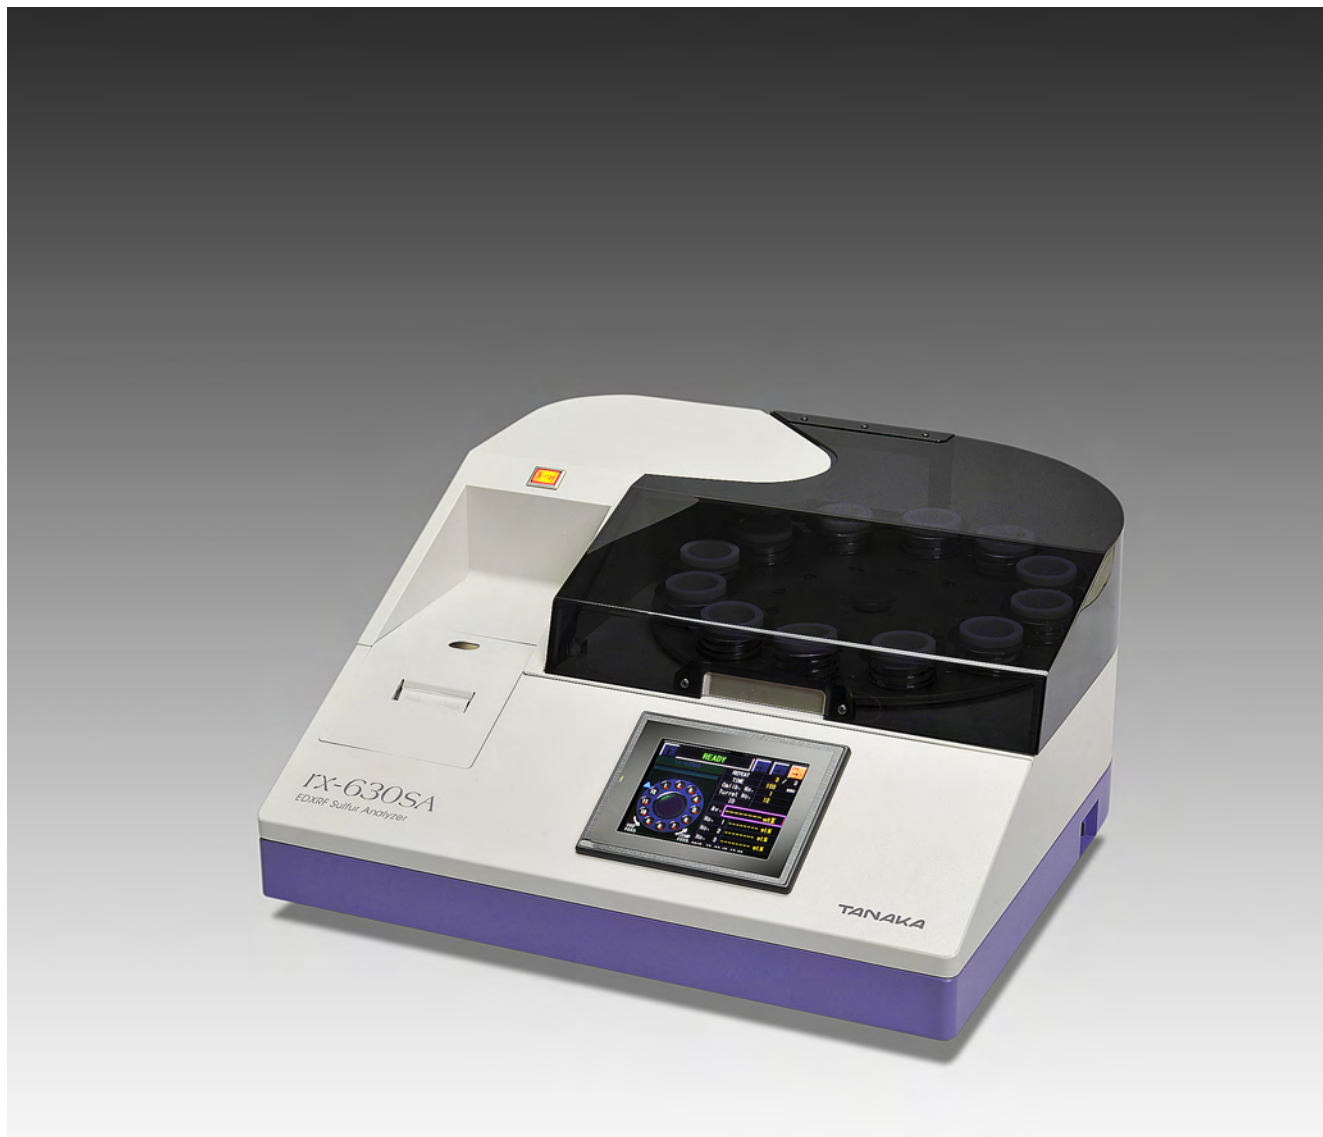

### Sample ID and data storage

By added Sample ID entering function, test result will be printed out with sample ID. rx-630SA has a data storage capability up to 999 test results and reprint previous data any time.

### Carousel type sample changer with acrylic cover

X-ray is shielded by a metallic cover moving downward on the objective sample cell. The acrylic cover is for dust protection of sample and measurement area, it may be opened during a test, allowing access to sample cells in the cue.

### Tool-free maintenance

By changing the fixed method of the carousel and the sample cell flange, sample leak protection sheet exchange can be done without using screw driver.

# EDXRF Sulfur Analyzer rx-630SA

## Specification

Test standard	ISO 8754, ASTM D4294 - 03, JIS K 2541 - 4, etc.
Sample	Kerosene, Naphtha, Gas oil, Crude oil, Base oil, etc.
Measuring range	0 to 6 wt%
Measuring time	10 to 990 sec, 1 to 99 times
Precision	LOD ( Limit of Detection ) = 15 mg/kg LOQ ( Limit of Quantitation ) = 50 mg/kg
Sample changer	Carousel type 12 - position ( sample volume : 3 to 5 ml )
X ray source	Small air - cooled X-ray tube rated 7 kv - 0.2 mA
X-ray detector	Gas-filled sealed proportional counter, long life type
Sample cell	Reusable 2- piece PTFE cup with disposable cell sheet
Automatic calibration	2 - Auto, 3 - Auto, M - Auto ( Max. 12 ) calibration
Automatic correction	C/H correction, Temperature correction, Barometric pressure correction.
Number of calibration curve	3
Printer	Built-in dot matrix type, paper width : 57 mm
Outlet	RS-232C × 1
Data storage	Last 999 test results
Safety	Cut off X-Ray tube power supply by interlock system when X-ray is leaked.
Installation site	10 to 30 °C ( with a temperature drift within 10 °C in a day ) Relative Humidity : Less than 80 %RH
Size ( W × D × H )	555 × 555 × 262 (mm)
Weight	27 kg
Power supply	AC 100 to 240 V 200 VA, 50 / 60Hz



## Standard accessories

AC Power Cord × 1  
 Sample Cell Holder × 12  
 Spring for Sample Cell Holder × 12  
 Sample Cell (PTFE Reusable) × 12  
 Jigs for Assembling / Disassembling Sample Cells × 1  
 Cell Sheet (200 mm × 1000 m) × 1  
 Sample Cell Stand × 1  
 Printing Roll Paper × 3  
 Spare Printing Ink Ribbon × 1

## Start up kit

Certified Reference Material

0.0 wt% , 100 mg/kg , 200 mg/kg , 500 mg/kg , 80 mg/kg , 0.1 wt% , 0.2 wt% , 0.5 wt% , 1 wt% , 2 wt% , 3 wt% and 4 wt%

Specifications subject to change without prior notice.

201608P